

{書類名} 図面

{図1}

Fig. 1A

(a)


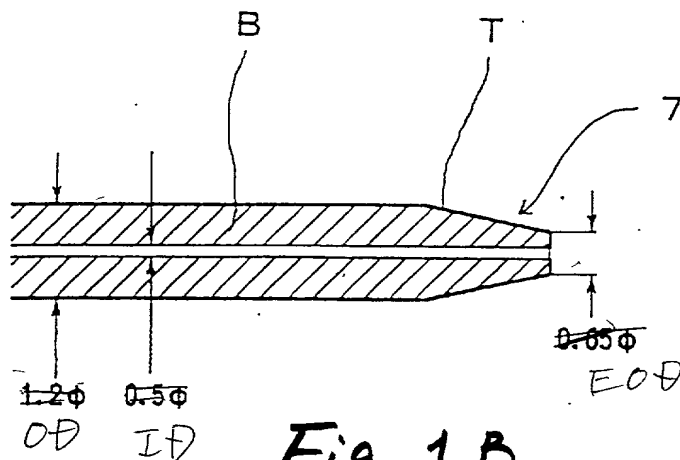


Fig. 1B

(b)

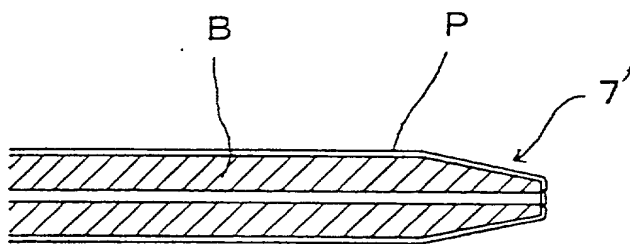

20056136-012403


【図2】

Fig. 2A

(a)

VIAL No. = 20

Injection amount
注入量: 2

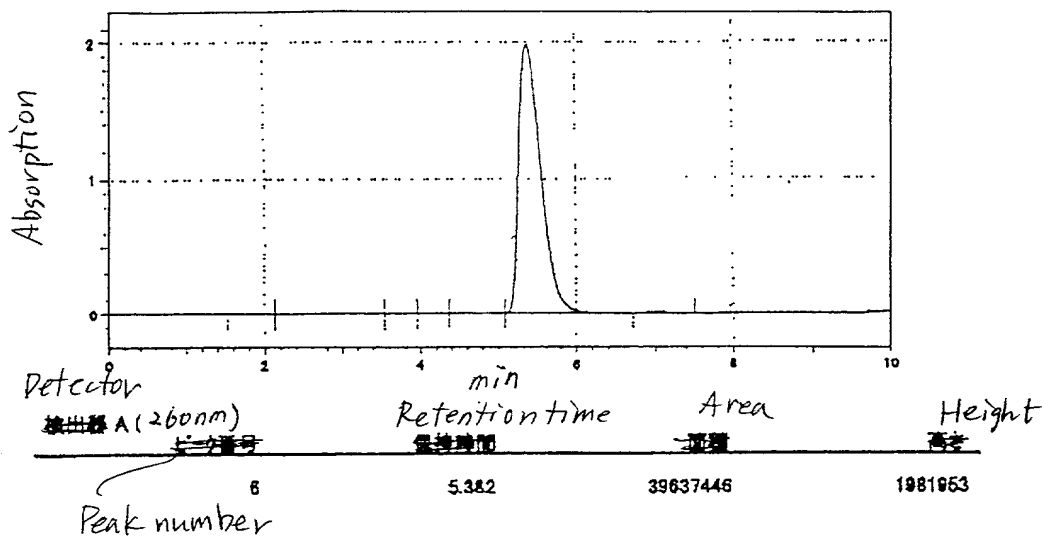


(b)

VIAL No. = 70

Injection amount
注入量: 2

Fig. 2B

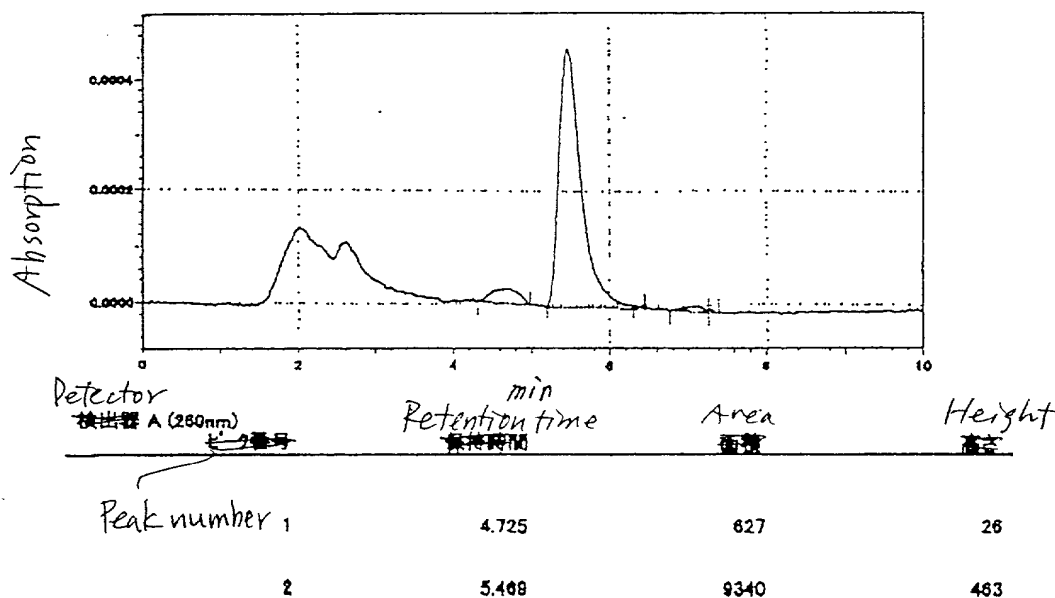

~~Fig. 3~~


Fig. 3A

~~(a)~~

VIAL No. = 10

注入量: 2

Injection amount

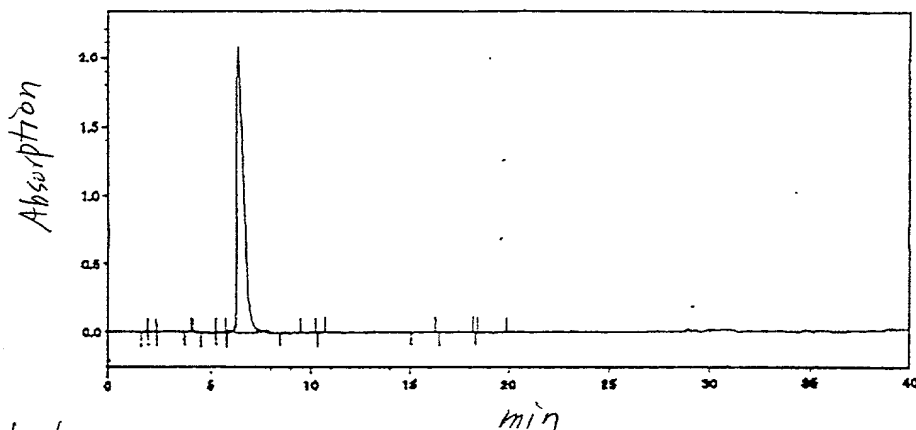

Detector

検出器 B (280nm)

Retention time

保持時間

6.525

Area

面積

48128387

Height

高さ

2067405


~~(b)~~

Fig. 3B

VIAL No. = 40

注入量: 2

Injection amount

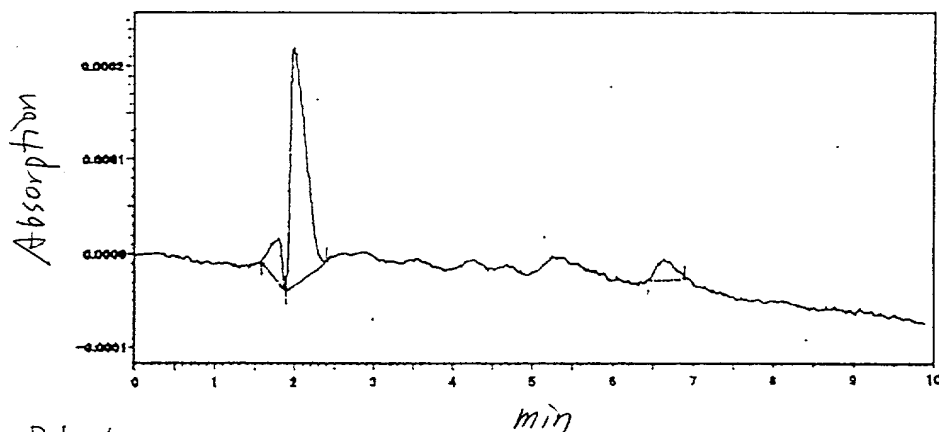

Detector

検出器 B (280nm)

Retention time

保持時間

6.553

Area

面積

321

Height

高さ

22

200503600001

【図4】

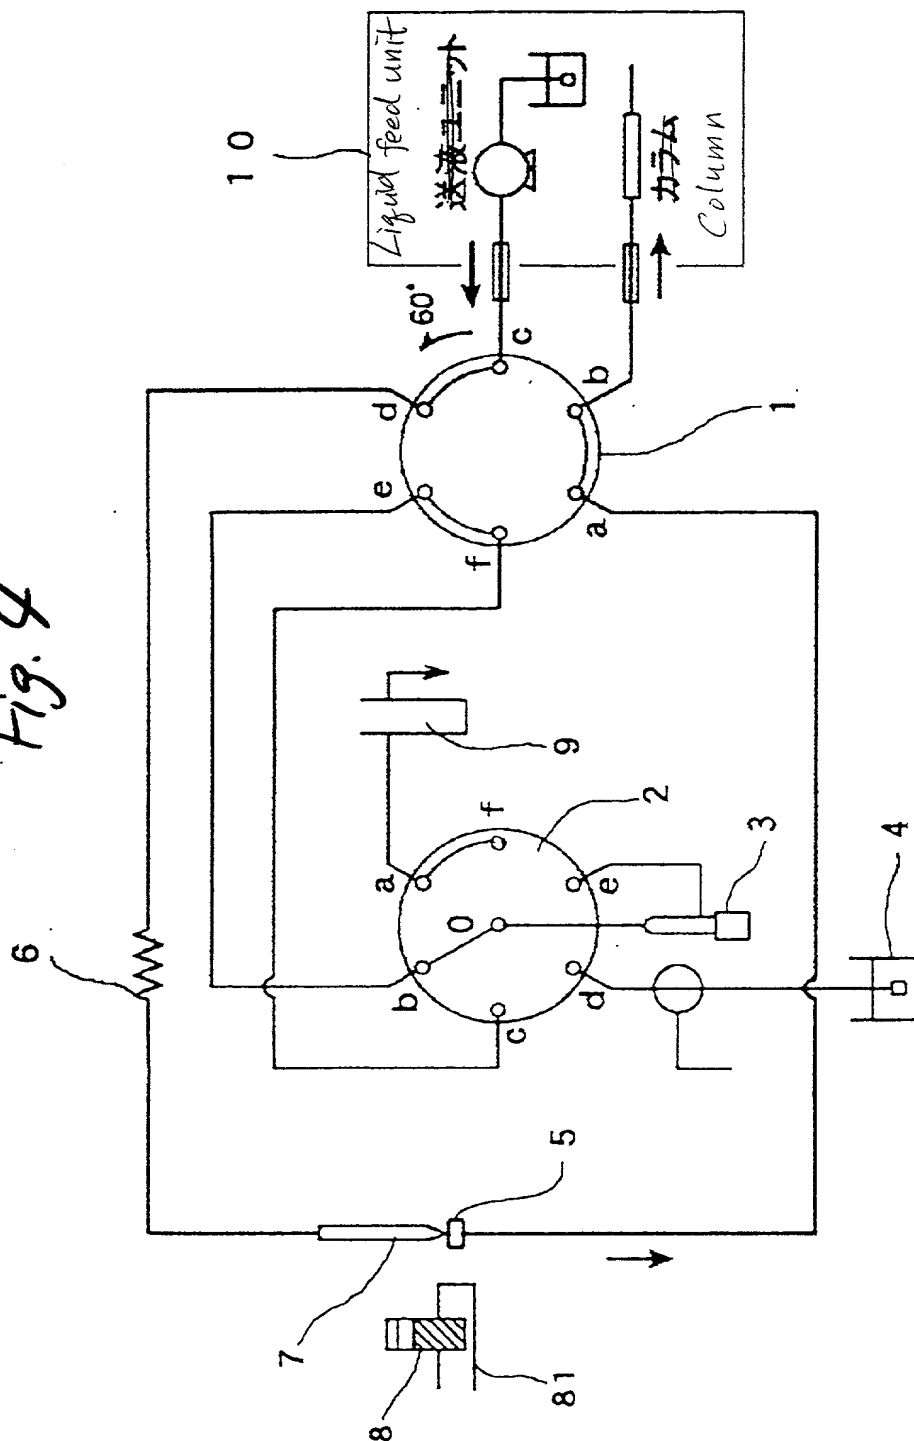


Fig. 4

204210-92195001